


PRONTO[®] APC kit

For the detection of the 3920T>A (I1307K) mutation in the APC gene

Instructions for Use

REF 9907



Tests



INTENDED USE

The PRONTO[®] APC kit is a Single Nucleotide Primer Extension Assay, determined by ELISA, intended for the qualitative *in vitro* detection of the 3920T>A (I1307K) mutation of the human APC gene in amplified DNA.

For *in vitro* diagnostic use.

BACKGROUND

Colon Cancer Predisposition

Autosomal dominant

Colorectal cancer (CRC) occurs in the colon (large intestine or bowel), rectum or anus. It is the second most common cancer in the USA usually striking after age 50. Approximately 130,000 cases of CRC are diagnosed in the USA each year and about 15% of these have a hereditary component. Early detection greatly increases the chances for a cure. Regular screening programs and early treatment have substantially reduced the death rate. A twofold increased lifetime risk for colorectal cancer is conferred by the I1307K mutation in the APC gene. This mutation creates a small hyper mutable region in the APC gene and indirectly leads to cancer predisposition. The I1307K mutation was found to be frequent (6%) among Ashkenazi Jews. Among patients with familial colon cancer of Ashkenazi origin, the mutation was present in 10-28% of the cases.

REFERENCES

1. *Nature Genet.*, 1997,17:79-83
2. *Gastroenterology*, 1999, 116: 54-57.

WARNINGS AND PRECAUTIONS

- Reagents supplied in this kit may contain up to 0.1% sodium azide that is toxic if swallowed. Sodium azide has been reported to form explosive lead or copper azides in laboratory plumbing. To prevent the accumulation of these compounds, flush the sink and plumbing with large quantities of water.

- TMB Substrate solution is an irritant of the skin and mucous membranes. Avoid direct contact.
- In addition to reagents in this kit, the user may come in contact with other harmful chemicals that are not provided, such as ethidium bromide and EDTA. The appropriate manufacturers' Material Safety Data Sheets (MSDS) should be consulted prior to the use of these compounds.

🔍 ASSAY OVERVIEW

The PRONTO[®] procedure detects predefined polymorphisms in DNA sequences, using a single nucleotide primer extension ELISA assay.

- 1 TARGET DNA AMPLIFICATION:** The DNA fragments that encompass the tested mutations are amplified. This amplified DNA is the substrate for the primer extension reaction.
- 2 POST-AMPLIFICATION TREATMENT:** The amplified DNA is treated to inactivate free unincorporated nucleotides, so that they will not interfere with the primer extension reaction.
- 3 PRIMER EXTENSION REACTION:** A single-nucleotide primer extension reaction is carried out in a 96-well thermoplate. Each well contains a 5'-labeled primer that hybridizes to the tested DNA next to the suspected mutation site, and a single biotinylated nucleotide species, which complements the nucleotide base at the tested site. Each post-amplification treated sample is tested in two wells per mutation: the first well of each pair tests for the presence of the mutant allele (*mut*), while the second well tests for the presence of the normal allele (*wt*). The biotinylated nucleotide will be incorporated to the primer in the course of the reaction or not added, depending on the tested individual's genotype.
- 4 DETECTION BY ELISA:** The detection of the biotinylated primers is carried out by an ELISA procedure: The biotin-labeled primers bind to a Streptavidin-coated ELISA plate and are detected by a peroxidase-labeled antibody (HRP) directed to the 5' antigenic moiety of the primer. A peroxidase reaction occurs in the presence of TMB-Substrate.
- 5 INTERPRETATION OF THE RESULTS:** Results are determined either visually (substrate remains clear or turns blue), or colorimetrically using the ELISA reader.

🔍 DISCLAIMER

- Results obtained using this kit should be confirmed by an alternative method.
- Confirmed results should be used and interpreted only in the context of the overall clinical picture. The manufacturer is not responsible for any clinical decisions that are taken.

The user of this kit should emphasize these points when reporting results to the diagnosing clinician or the genetic counselor.

🔍 CONTENTS OF THE KIT

APC Amplification Mix	1 x vial (clear cap)	(1.2mL)
PRONTO [®] Buffer 2	1 x bottle	(3 mL)
Solution C	1 x vial (yellow cap)	(130 µL)
Solution D	1 x vial (red cap)	(100 µL)
ColoRed TM -Oil	1 x dropper bottle	(13 mL)
Assay Solution	1 x bottle (green solution)	(100 mL)
Wash Solution (conc. 20x).....	1 x bottle	(100 mL)
Conjugated HRP (conc. 100x) ..	1 x vial	(450 µL)
TMB- Substrate	1 x bottle	(40 mL)
PRONTO [®] APC Plates	2 x individually pouched plates	
Detection Plates	2 x Streptavidin-coated ELISA plates	

🔍 STORAGE AND STABILITY

- Store at 2-8°C. Do not freeze.
- Do not use the kit beyond its expiration date (marked on box label). Stability is maintained even when components are re-opened several times.
- Minimize the time reagents spend at room temperature.
- This kit has been calibrated and tested as a unit; **do not mix reagents from kits with different lot numbers.**

🔍 ADDITIONAL MATERIALS REQUIRED

- Taq DNA polymerase
- Deionized water (about two liters per kit)
- Thermowell plate or tubes (thin wall) for the post-amplification treatment
- Sterile pipette tips
- Troughs / reagent reservoirs - for use with the detection reagents
- Thermocycler for a 96-well microplate
- Multichannel pipettes (5-50 µL and 50-200 µL)
- Positive displacement pipettes (1-5 µL, 5-50 µL, 50-200 µL and & 200-1,000 µL)
- Filtered tips
- ELISA reader with a 620 nm filter
- Polaroid camera and color film to record results (optional)
- Automated microtiter plate washer or squirt bottle
- Vortex mixer
- Timer

ASSAY PROCEDURE

1 DNA AMPLIFICATION

1. **Dispense** 2 µL template DNA (from an initial concentration of about 150 ng/µL) to a thermoplate well or tube.
2. **Prepare** a Master Mix in a sterile vial, according to the volumes indicated in the table below, plus one spare reaction volume. Add the Taq DNA polymerase to the Master Mix shortly before dispensing the Mix. Gently mix by pipetting in and out several times.

Master Mix

Solution	Volume for one sample
Amplification mix APC	13.0 µL
Taq DNA Polymerase (5 u/µL)	0.25 µL

The following Taq DNA polymerases were validated for use with this procedure (lacking 3' → 5' exonuclease activity):

- PHARMACIA Cat. # 27-0799
- SIGMA Cat. # D-1806
- ROCHE Cat. # 1-146-165
- PROMEGA Cat. #. M-1661
- BIOLINE Cat. # M95801B
- PERKIN ELMER Cat. # M801-0060

3. **Dispense** 13 µL Master Mix to each well or tube.
4. **Add** one drop of ColoRed™ oil to each well. Do not touch the wells with the tip of the oil bottle. Even when using a thermocycler with a hot lid, it is essential to use oil.
5. **Place** the thermoplate well or tube in a thermocycler previously programmed with the following protocol:

Cycling Protocol		
1.	94°C	2 minutes
2.	94°C	30 seconds
3.	53°C	30 seconds
4.	72°C	30 seconds
5.	72°C	5 minutes

} 35 cycles

6. To verify amplification, subject 5 µL of the amplified product to electrophoresis in a 2% agarose gel. The size of the APC gene amplified fragment is 290 bp.

Limitation of the test:

Different Taq DNA polymerases and thermocyclers may influence the amplification yield dramatically. It is recommended to use a validated Taq DNA polymerase and a calibrated thermocycler.

2 POST-AMPLIFICATION TREATMENT

1. **Prepare** a post-amplification mix shortly before use. Combine in a single test tube PRONTO[®] buffer 2, Solution C and Solution D according to the volumes appearing in the following table. Multiply the volume by the number of tested samples, plus one spare volume.

Post-Amplification Mix

Solution	Volume for one sample
PRONTO [®] Buffer 2	15.0 µL
Solution C	0.7 µL
Solution D	0.5 µL

2. **Mix** gently by pipetting this solution in and out five times. **Do not vortex.**
3. **Dispense** 15 µL of the post-amplification mix into each thermowell plate well or tube containing 10 µL of the amplified DNA.
Ensure that the solution you add becomes well mixed with the DNA sample by pipetting.
4. **Add** one drop of ColoRed[™] oil to each tube. Do not touch the tube with the tip of the oil bottle. Even when using a thermocycler with a hot lid, it is essential to use oil.
5. **Incubate** for 30 minutes at 37°C, then for 10 minutes at 95°C in a thermocycler.

If not used immediately, the treated sample can be kept at 2-8°C for a maximum of 4 hours.

3 PRIMER EXTENSION REACTION


1. **Program** the Thermocycler to the following protocol:

Cycle	Temperature	Time
Start:	94°C	15 sec.
20 cycles:	94°C	30 sec.
	60°C	10 sec.
End:	18°C - 25°C (Cool down to room temperature)	

2. **Take** a PRONTO[®] Plate out of its pouch. Notice the color at the bottom of the wells. For each mutation tested, use a pink well (*mut*) and a blue well (*wt*). Mark the plate with the ID numbers of your test.
If you intend to use less than a full plate, you can cut the plate and return the unused portion to the pouch. If you do this, seal the pouch immediately with its desiccant card inside.
3. **Dispense** 8 µL of post-amplification treated DNA into the first two wells in row A (see Fig. 1). Continue with the remaining samples. It is possible to transfer up to eight samples simultaneously using a multichannel pipette.

Ensure that the solution is at the bottom of each well by inspecting the plate from below. Be sure that the well does not contain air bubbles.

Figure 1: Dispensing of the Post-Amplified DNA into the PRONTO[®] APC Plate

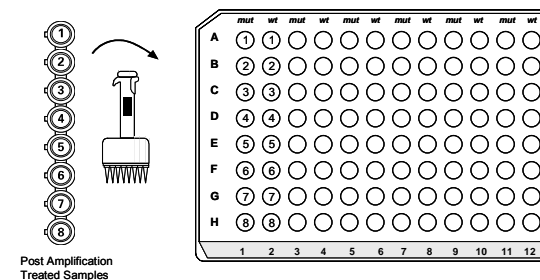

Recommendation:

Use a new set of tips for each column. Alternatively use the same set of tips, but do not touch the bottom of the wells.

- 4 Tilt the plate and add one drop of ColoRed™ oil to each well. Do not touch the well with the tip of the oil bottle. Even when using a thermocycler with a hot lid, it is essential to use oil.
- 5 Turn on the thermocycler and start the cycling protocol.
- 6 When the thermal cycling is complete, you can proceed to the ELISA assay, or store the reaction products in the refrigerator and carry out the visualization steps within 24 hours.

4 ELISA ASSAY - COLOR DEVELOPMENT

The ELISA assay consists of the following steps:

1. **Binding** the biotin-labeled extended primers to the Streptavidin-coated plate.
2. **Washing** away unbound primers.
3. **Incubating** with the HRP conjugate.
4. **Washing** away unbound conjugate.
5. **Incubating** with the TMB Substrate (color development).

The results of this assay can be determined in one of two ways:

- a Visually:** by monitoring the development of the blue color.
- or
- b Colorimetrically:** by measuring the absorbance, using an ELISA reader at a wavelength of 620 nm.


PREPARATION

- All components used in the detection step should reach room temperature before starting the assay.
- **Dilute** the 20x Wash Solution to 1x with deionized water.
Dilute solution may be kept at 18-25°C for up to one month.
- **Peel** off the plastic cover of the Detection Plate. Mark the side of the plate with the kit name and test number.
- **Place** the PRONTO® Plate and the Detection Plate side by side, oriented in the same direction (see Fig. 2).

TRANSFER TO THE DETECTION PLATE

1. Fill a reagent reservoir / trough with the green colored Assay Solution. About 11 mL will be required for a 96-well plate.
2. Using a multichannel pipette **add** 100 µL of Assay Solution to the bottom of each well in column 1 of the PRONTO® Plate. Gently mix by pipetting in and out 3-4 times.
3. **Without changing tips, transfer** 100 µL from each well in this column to the first column in the Detection Plate (see Fig. 2).
Ensure that the solution at the bottom of all wells of the PRONTO® Plate has turned green by inspecting them from below.

Figure 2: Transferring the Primer Extension Products from the PRONTO® Plate to Detection Plate.

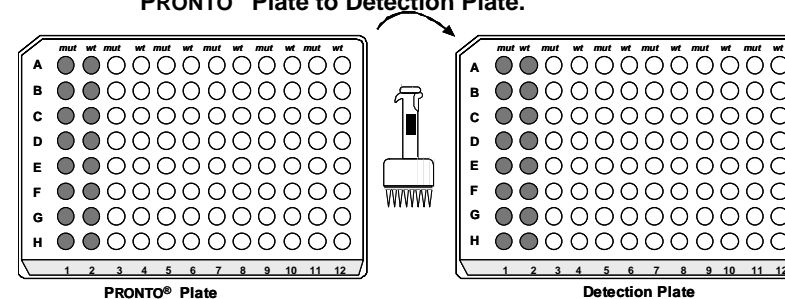

4. **Repeat** this procedure using a new set of tips for each remaining column. It is important to maintain the order of the samples.
Note: 10 μ L of oil carried over or 10 μ L of the sample left behind will not significantly affect the detection process.
5. **Incubate** for 10 minutes at RT (18-25°C).
6. While the incubation takes place, **dilute** the Conjugated HRP 1:100 in Assay solution (green solution). About 11 mL are needed for a 96-well Plate. This solution must be freshly prepared each time the test is run.
7. **Empty** the plates, **wash** four times with 350 μ L 1x Wash Solution. Ensure that the plates are dry after the last wash step.
8. With a multichannel pipette add 100 μ L **freshly-diluted** Conjugated HRP to all the wells.
9. **Incubate** for 10 minutes at RT.
10. **Wash** as in step 7.
11. **Add** 100 μ L TMB substrate to each well with a multichannel pipette and incubate for 15 minutes at RT (18-25°C) until the blue color appears sufficiently strong (15 minutes).
12. For Visual Detection: Results may be documented by a standard Polaroid camera with color film (for example – Fuji FP-100C).
13. For Colorimetric Detection: **Agitate** the plate gently to homogenize the color in the wells. **Read** the results in an ELISA reader using a 620 nm filter (single wavelength setting).

VALIDATION OF THE RESULTS


For Visual Detection:

For every mutation site tested, at least one of the wells should develop a deep blue color. Otherwise, results are invalid for the relevant mutation (see Fig. 3).

For Colorimetric Detection:

For every mutation site tested, at least one of the two wells should yield an O.D ≥ 0.50 .

Figure 3: Visual Interpretation of Genotypes

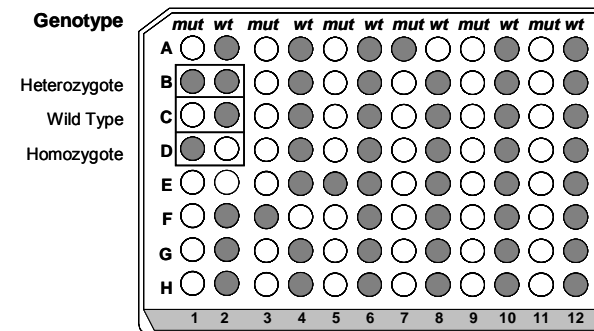


INTERPRETATION OF RESULTS

Important: Heterozygous or homozygous mutant results should be confirmed by retesting. It is recommended to repeat the test with newly extracted DNA.

Criteria for Visual Interpretation

A deep blue color indicates positive signal, while negative signals appear as a clear to pale blue well (see Fig. 4).

Figure 4: Genotype assignment according to visual inspection of test results

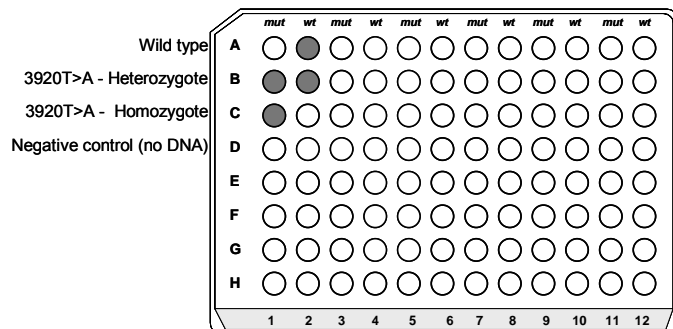

Criteria for Colorimetric Interpretation (O.D. 620)

The genotype of each sample is determined according to two criteria:

- The O.D. values of the *mut* and *wt* wells.
- The ratio of *mut/wt* O.D. values.

Calculate the *mut/wt* ratios by dividing the signal of the *mut* well by the signal of the *wt* well.

Identify the correct genotype of each mutation using the table below:

Genotype	<i>mut</i> well	<i>wt</i> well	<i>mut/wt</i> ratio
Normal	O.D. ≤ 0.35	O.D. ≥ 0.5	ratio ≤ 0.5
Heterozygote	O.D. ≥ 0.5	O.D. ≥ 0.5	$0.5 \leq \text{ratio} \leq 2.0$
Homozygote	O.D. ≥ 0.5	O.D. ≤ 0.35	ratio ≥ 2.0

! Samples with values not included in the above table are considered indeterminate and should be retested.

PRONTO® APC – PROCEDURE SUMMARY

DNA EXTRACTION: from human whole blood, using a validated method.

DNA AMPLIFICATION:
Volumes per reaction: 2 μ L Template DNA + 13 μ L Amplification Mix + 0.25 μ L Taq Polymerase.
Cycling protocol: 94°C 2 min \rightarrow 35 cycles of {94°C 30 sec. / 53°C 30 sec. / 72°C 30 sec.} \rightarrow 72°C 5 min.

POST-AMPLIFICATION PROCEDURE:

- Volumes per reaction:

PRONTO® Buffer 2	15.0 μ L
Solution C	0.7 μ L
Solution D	0.5 μ L
- Pipette in and out to mix.
- Add 15 μ L into each well containing 10 μ L amplified DNA sample and mix well.
- Top with one drop of ColoRed™ Oil.
- Incubate 30 minutes at 37°C, then 10 minutes at 95°C.

PRIMER EXTENSION REACTION:

- Dispense 8 μ L of each post-amplification treated DNA into two wells of the PRONTO® Plate.
- Top off with one drop of ColoRed™ Oil.
- Start the cycling protocol:
94°C 15 sec \rightarrow 20 cycles of {94°C 30 sec. / 60°C 10 sec.} \rightarrow Cool.

Insert the PRONTO® Plate in the thermocycler when the temperature has reached 90°C

DETECTION:

- Add 100 μ L Assay Solution to each well in the PRONTO® Plate and mix.
- Transfer 100 μ L from each well of the PRONTO® Plate to the respective position in the Detection Plate. Incubate 10 minutes at RT.
- Empty the wells and wash four times with 350 μ L of 1x Wash Solution.
- Add 100 μ L 1:100 Conjugate HRP to every well; incubate for 10 minutes at RT.
- Wash the wells again.
- Add 100 μ L Substrate to each well; incubate at RT for 15 minutes.

For troubleshooting guide, please refer to our website:

www.prontodiagnosics.com

PRONTO is a Registered Trademark.

2 GENESCREEN and COLORED are Trademarks of Pronto Diagnostics.

Copyright © 2005 Pronto Diagnostics Ltd.

The PRONTO® Technology is covered by US patent 5,710,028, by European patent 0648222 and by corresponding national patents.

Produced by Pronto Diagnostics Ltd.

Kiryat Atidim

Building 3, 3rd floor

POB 58129

Tel Aviv 6158002

Israel

Tel: +972.73.2126155

Fax: +972.73.2126144

Customer Service: E-Mail: info@prontodiagnosics.com

Authorized EU Representative:

MedNet GmbH,

Borkstrasse 10, 48163 Münster,

Germany

Tel: +49.251.32266-0

Fax: +49.251.32266-22

MC9907 09.EN.02